

# Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

## Optical Fiber Diameter Analyser (OFDA100) Micron Test Report

Pohopoco Creek Alpacas/Mary Baxter  
216 Merwinsburg Rd  
Effort PA 18330-7817 USA

06/15/15

Test No: 903437


### Animal and Sample Description

**Animal Name:** Pohopoco Creek's Spot  
**Breed:** Alpaca(Huacaya)  
**Sex:** Male  
**Color:** White

**Animal ID:** 32464818  
**Sample Location:** Side  
**Sample Date:** 05/10/15  
**Age:** 09/29/12

### Laboratory Data

<b>Mean Fiber Diameter:</b>	23.0 microns	<b>Spin Fineness:</b>	22.0 microns
<b>Standard Deviation:</b>	4.3 microns	<b>Mean Curvature (deg/mm):</b>	30.6
<b>Coefficient of Variation:</b>	18.8 %	<b>SD Curvature (deg/mm):</b>	18.4
<b>Fibers Greater Than 30 microns:</b>	5.7 %	<b>Comfort Factor:</b>	94.3 %

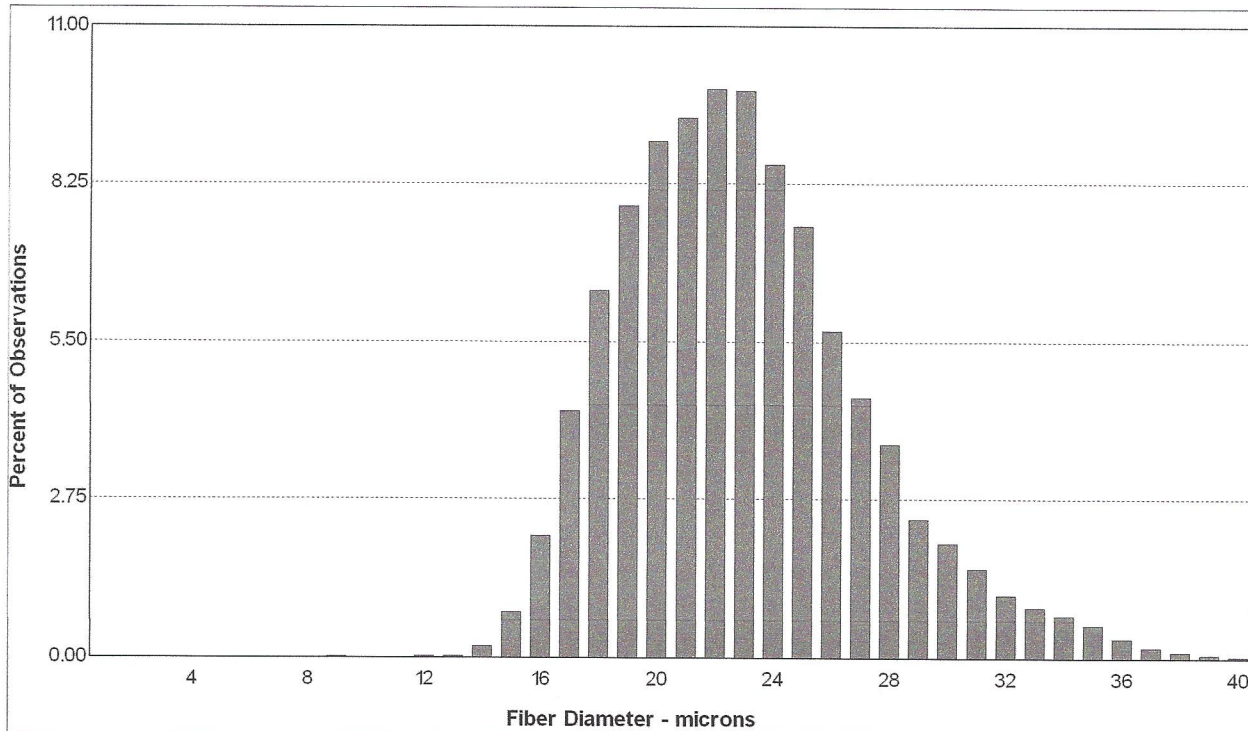

This Test Performed According to I.W.T.O Method 47